

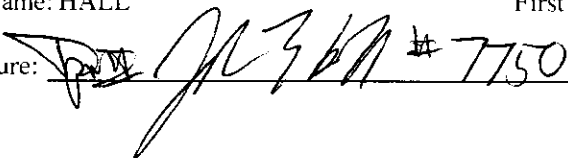
Alcotest 7110 Calibration Record


Equipment


Alcotest 7110 MKIII-C	Serial No.: ARUM-0043	
Location: CHERRY HILL TWSP. P.D.		
Calibration File No.: 02911	Calib. Date: 04/23/2024	Calib. No.: 00049
Certification File No.: 02871	Cert. Date: 08/15/2023	Cert. No.: 00042
Linearity File No.: 02872	Lin. Date: 08/15/2023	Lin. No.: 00043
Solution File No.: 02910	Soln. Date: 03/29/2024	Soln. No.: 00395
Sequential File No.: 02911	File Date: 04/23/2024	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDWA S3-0007
Control Solution %: 0.100%		Expires: 07/05/2024
Solution Control Lot: 22240		Bottle No.: 1186

Coordinator

Last Name: HALL First Name: JOSHUA MI: B

Signature:  # 7750 Badge No.: 7750 Date: 04/23/2024

*Black Key Temperature Probe Serial.....# DOEE P2-081 

*Digital NIST Temperature Measuring System Serial.....# 230 208 368 

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02911	Calib. Date:	04/23/2024
Certification File No.:	02912	Cert. Date:	04/23/2024
Linearity File No.:	02872	Lin. Date:	08/15/2023
Solution File No.:	02910	Soln. Date:	03/29/2024
Sequential File No.:	02912	File Date:	04/23/2024
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWA S3-0007
Solution Control Lot:	22240	Expires:	07/05/2024
		Bottle No.:	1186

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:14D		
Control 1 EC	0.099%	13:15D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		
Control 2 EC	0.099%	13:16D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 3 EC	0.099%	13:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18D		


All tests within acceptable tolerance.

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 04/23/2024

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0043
Location:	CHERRY HILL TWSP. P.D.		
Calibration File No.:	02911	Calib. Date:	04/23/2024
Certification File No.:	02912	Cert. Date:	04/23/2024
Linearity File No.:	02913	Lin. Date:	04/23/2024
Solution File No.:	02910	Soln. Date:	03/29/2024
Sequential File No.:	02913	File Date:	04/23/2024
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.040%	Serial No.:	DDWF S3-0237
Solution Control Lot:	22250	Expires:	07/19/2024
		Bottle No.:	1235
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.080%	Serial No.:	DDWF S3-0242
Solution Control Lot:	22270	Expires:	07/28/2024
		Bottle No.:	0445
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.160%	Serial No.:	DDWF S3-0218
Solution Control Lot:	22290	Expires:	08/04/2024
		Bottle No.:	0121

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:35D		
Control 1 EC	0.040%	13:36D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	13:36D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:37D		
Control 2 EC	0.040%	13:38D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	13:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:39D		
Control 3 EC	0.080%	13:40D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	13:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41D		
Control 4 EC	0.080%	13:42D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	13:42D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:43D		
Control 5 EC	0.159%	13:44D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.158%	13:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:46D		
Control 6 EC	0.159%	13:46D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.157%	13:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:48D		

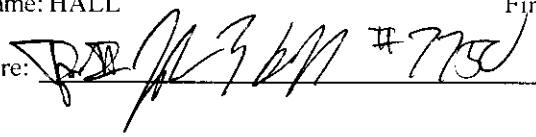
All tests within acceptable tolerance.

Coordinator

Last Name: HALL

First Name: JOSHUA

MI: B

Signature: 

Badge No.: 7750

Date: 04/23/2024

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02870 Calib. Date: 08/15/2023 Calib. No.: 00046
Certification File No.: 02871 Cert. Date: 08/15/2023 Cert. No.: 00042
Linearity File No.: 02872 Lin. Date: 08/15/2023 Lin. No.: 00043
Solution File No.: 02906 Soln. Date: 11/24/2023 Soln. No.: 00394
Sequential File No.: 02906 File Date: 11/24/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWA S3-0008
Control Solution %: 0.100% Expires: 06/05/2025
Solution Control Lot: 23200 Bottle No.: 1057

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:19S		
Control 1 EC	0.099%	10:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		
Control 2 EC	0.098%	10:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22S		
Control 3 EC	0.098%	10:23S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:23S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

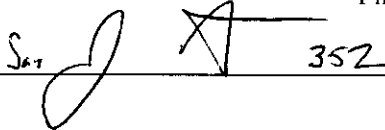
Changed By:

Last Name: WEIST

First Name: JAMES

MI: R

Signature: _____

 352

Badge No.: 352

Date: 11/24/2023

Calibrating Unit

New Standard Solution Report


Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0043
Location: CHERRY HILL TWSP. P.D.
Calibration File No.: 02911 **Calib. Date:** 04/23/2024 **Calib. No.:** 00049
Certification File No.: 02912 **Cert. Date:** 04/23/2024 **Cert. No.:** 00043
Linearity File No.: 02913 **Lin. Date:** 04/23/2024 **Lin. No.:** 00044
Solution File No.: 02914 **Soln. Date:** 04/23/2024 **Soln. No.:** 00396
Sequential File No.: 02914 **File Date:** 04/23/2024

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDWA S3-0007
Control Solution %: 0.100% **Expires:** 06/05/2025
Solution Control Lot: 23200 **Bottle No.:** 1256

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:56D		
Control 1 EC	0.100%	14:56D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:56D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57D		
Control 2 EC	0.100%	14:58D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:58D		
Control 3 EC	0.100%	14:59D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	14:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUJ P2 - 158 GBK
Changed By:
Last Name: HALL **First Name:** JOSHUA **MI:** B
Signature:  #7750 **Badge No.:** 7750
Date: 04/23/2024

Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings

Coordinator:

Tpr. II Joshua B. Hall
Name

7750
Badge No.

Location:

Cherry Hill Twp. P.D.
Agency

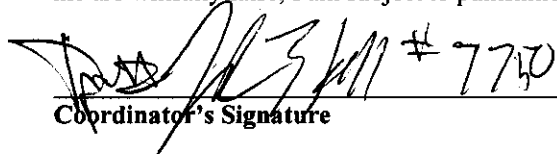
ARUM-0043
Alcotest Serial No.

Equipment:

230 208 368
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDWF S3-0237	11:58 D	12:59 D	33.9°C
0.08%	DDWF S3-0242	11:58 D	13:00 D	33.9°C
0.10%	DDWA S3-0007	11:58 D	13:01 D	33.9°C
0.16%	DDWF S3-0218	11:58 D	13:02 D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

 # 7750
Coordinator's Signature

04/23/2024
Date

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDWFS3-0237

Certification Date:

12-2-23

Technician:

DH / CR

Re-Certification Due Date:

12-2-24

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDWFS3-0242

Certification Date:

12-20-23

Technician:

DH / CR

Re-Certification Due Date:

12-20-24

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDWF 53-0218

Certification Date:

12-2-23

Technician:

DH / CR

Re-Certification Due Date:

12-2-24

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-081

Certification Date:

12-5-23

Next Certification Due:

12-5-24

Probe Value:

104

Draeger, Inc.

DH / CR



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-14045052

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 230208368

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A42238		
PRT Temperature Probe	02022	13 Dec 2023	4500022592
Temperature Probe	5357	01 Jul 2023	4500015492
Thermistor Module	B5C344	20 Jun 2023	1000481112
Temperature Calibration Bath	B93537		
Thermistor Module	B96381	23 Aug 2023	1000483176
Temperature Probe	5392	06 Sep 2023	4500018330
Temperature Probe	5398	06 Sep 2023	4500018329
Digital Thermometer	B96088	10 Mar 2024	1000489962

Certificate Information:

Technician: 420

Procedure: CAL-06

Cal Date: 27 Mar 2023

Cal Due Date: 27 Mar 2025

Test Conditions: 57.99%RH 23.66°C 1013mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		-0.002	0.001	Y	-0.052	0.048	0.0087	>4:1
°C	N.A.	N.A.		25.002	25.003	Y	24.952	25.052	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.003	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.002	99.998	Y	99.952	100.052	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio;
Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Jenny Ren

Jenny Ren, Technical Manager

Note:

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be effected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-14045052

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 27 Mar 2023

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01806-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS **0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 08/08/2024

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 24260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1218 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 23, 2026.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of August, 2024.

[Signature]
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS **0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 07/18/2023

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 23200

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1219 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 5, 2025.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 19 day of July, 2023.

Notary 

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/21/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1205 to 0.1219 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 05, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 27 day of July, 2022.
[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110022
My Commission Expires 0/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 05/23/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22160


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 9, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 26 day of May, 2022.


Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110822
My Commission Expires 01/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 04/26/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22110

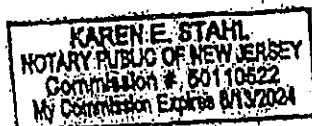
Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1219 to 0.1237 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 4, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Acting OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of April, 2022.
[Signature]
Notary



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 04/26/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22110

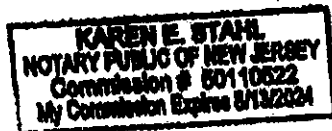
Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1219 to 0.1237 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 4, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Acting OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of April, 2022.
[Signature]
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHELLEY Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 05/23/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22160

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 9, 2024.

As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 26 day of May, 2022.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 01/3/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 08/17/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0483 grams per 100 milliliters of solution.

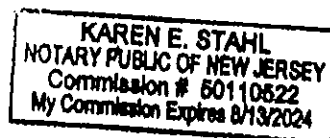
This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

Notary 



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/18/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0967 to 0.0983 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 28, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Prohibited from Racially Profiling and Bias Incidents





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

CERTIFICATION OF ANALYSIS 0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/22/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1924 to 0.1948 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 4, 2024.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 9 day of September, 2022.
[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Joshua B. Hall

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 141 OF

THE LAWS OF THE STATE OF NEW JERSEY, ALCOHOL 710 MKIII-C

A METHOD TO DETERMINE INTOXICATION

ON THE 29th DAY OF March

TWO THOUSAND AND TWENTY TWO

[Signature] *[Signature]*

COLUMBIA COLLEGE ACTING ATTORNEY GENERAL
NEW JERSEY STATE POLICE STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 12/22)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Joshua B. Hall

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 141 OF

THE LAWS OF THE STATE OF NEW JERSEY, ALCOHOL 710 MKIII-C

A METHOD TO DETERMINE INTOXICATION

ON THE 21st DAY OF December

TWO THOUSAND AND SEVENTEEN

[Signature] *[Signature]*

ACTING SUPERINTENDENT ATTORNEY GENERAL
NEW JERSEY STATE POLICE STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 8/22/19	NTSP Gallwey	B. A.
2. 1/12/21	ACCX	B. A.
3. 10-3-23	ACCX	B. A.
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 11/17)



Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

03/29/2024

ARUM-0043

Draeger, Inc.



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

Ø Model: ALCOTEST CU34

○ Model: MARK IIA

○ X-Cal 2000 (Alcosim)

○ Other: _____

Serial Number:

DDWA S3-0007

Certification Date:

10-23-23

Technician:

DH / CR

Re-Certification Due Date:

10-23-24

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DD4JP2-158

Certification Date:

10-23-23

Next Certification Due:

10-23-24

Probe Value:

106

Draeger, Inc.

DH / CR



NEW JERSEY STATE POLICE
Alcohol Drug Testing Unit

Tpr. II Joshua B. Hall #7750

Hamilton Technology Complex
Suite #400
1200 Negron Drive
Hamilton, NJ 08691

Tel#: (609) 584-5051 ext 5608
Email: Joshua.Hall@njsp.gov
Cell# (609) 947-3179